



10/796,645
Malek et al.
Mass Spectrometer

1 / 7

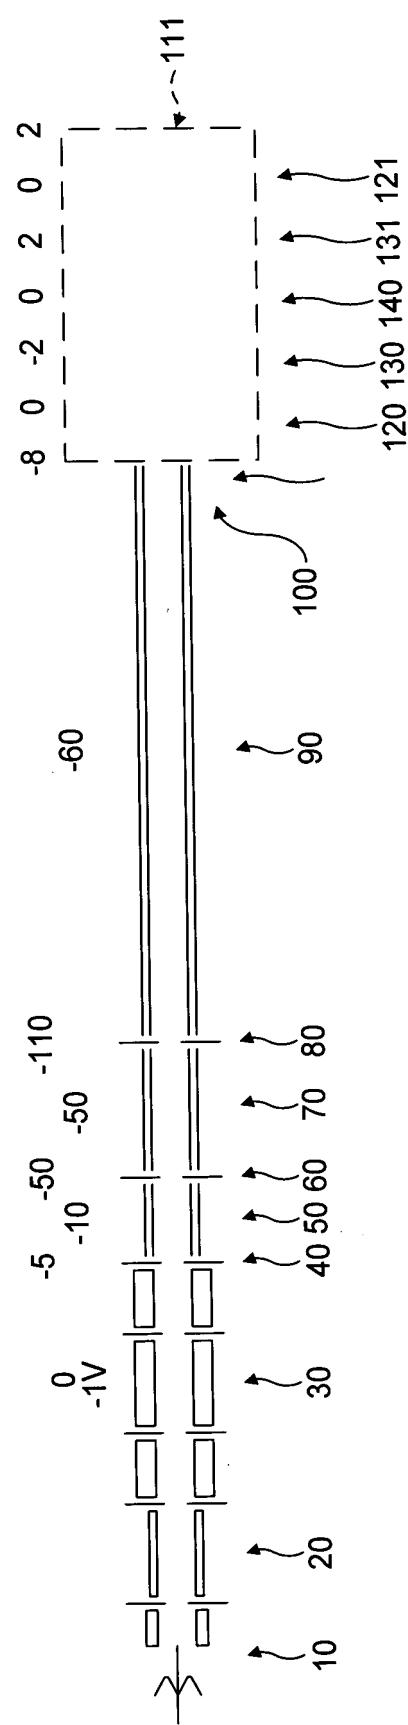


FIG. 1

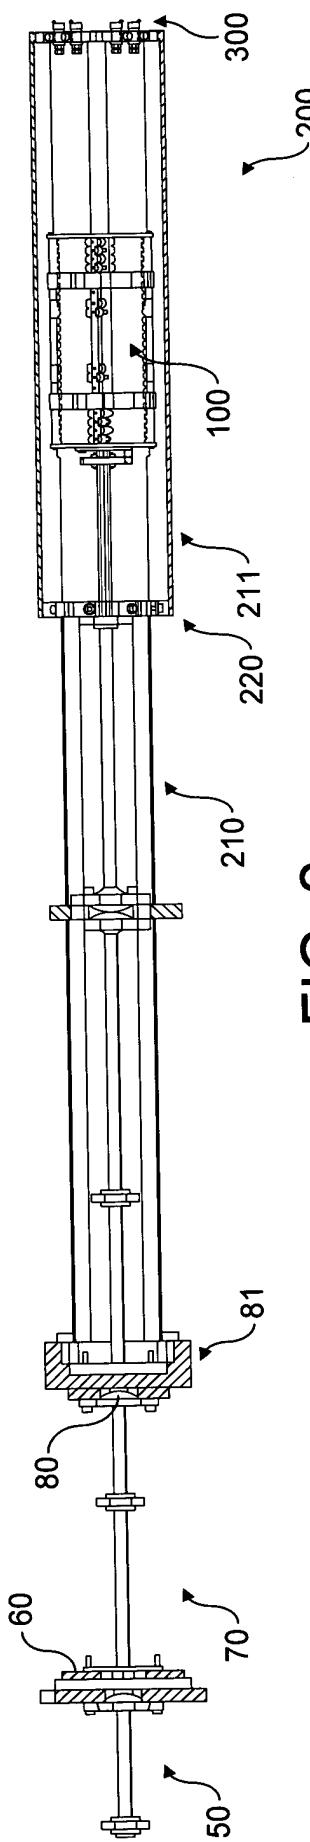


FIG. 2a

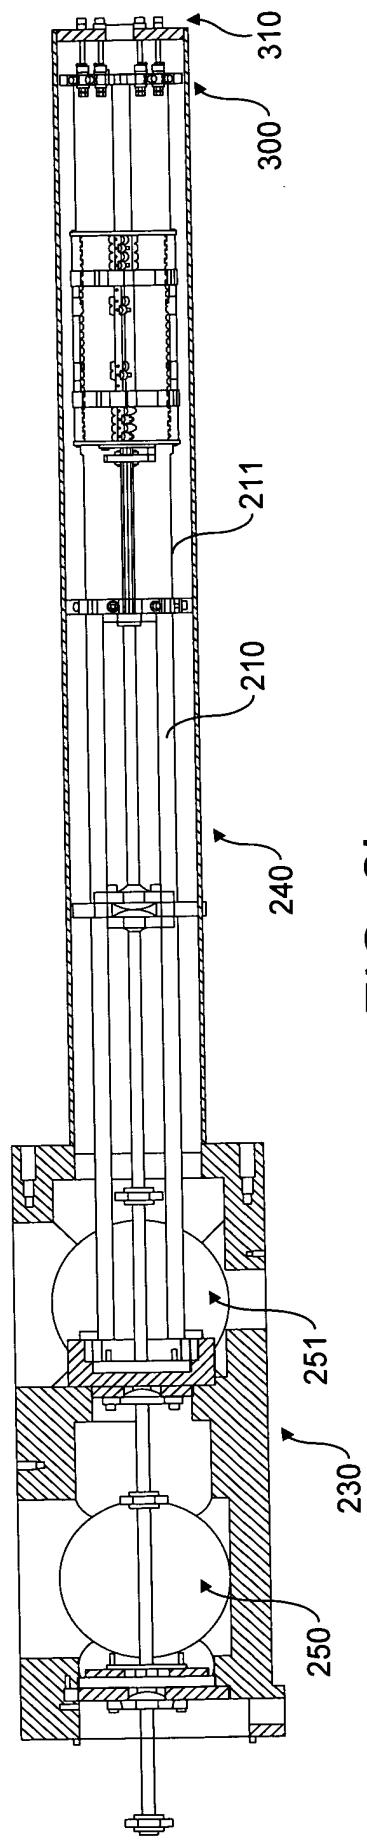


FIG. 2b

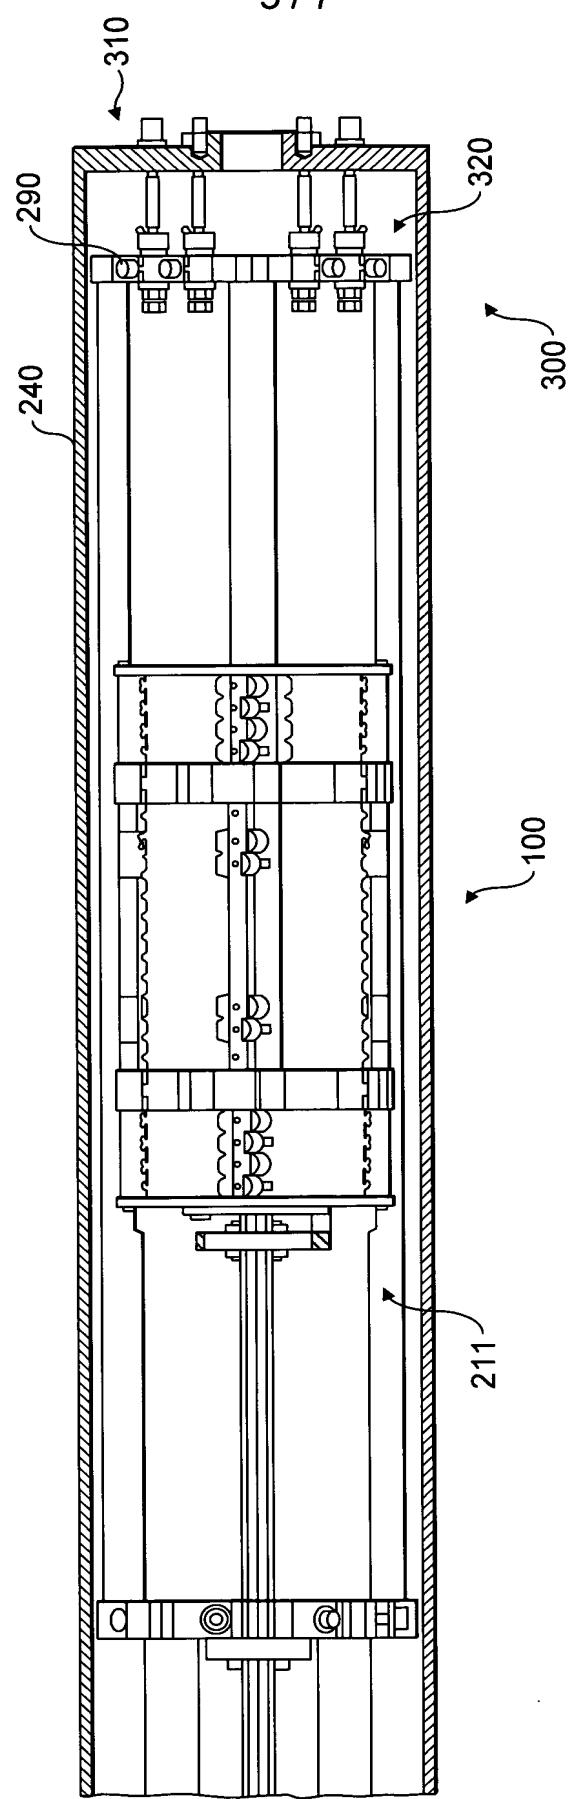


FIG. 3

4 / 7

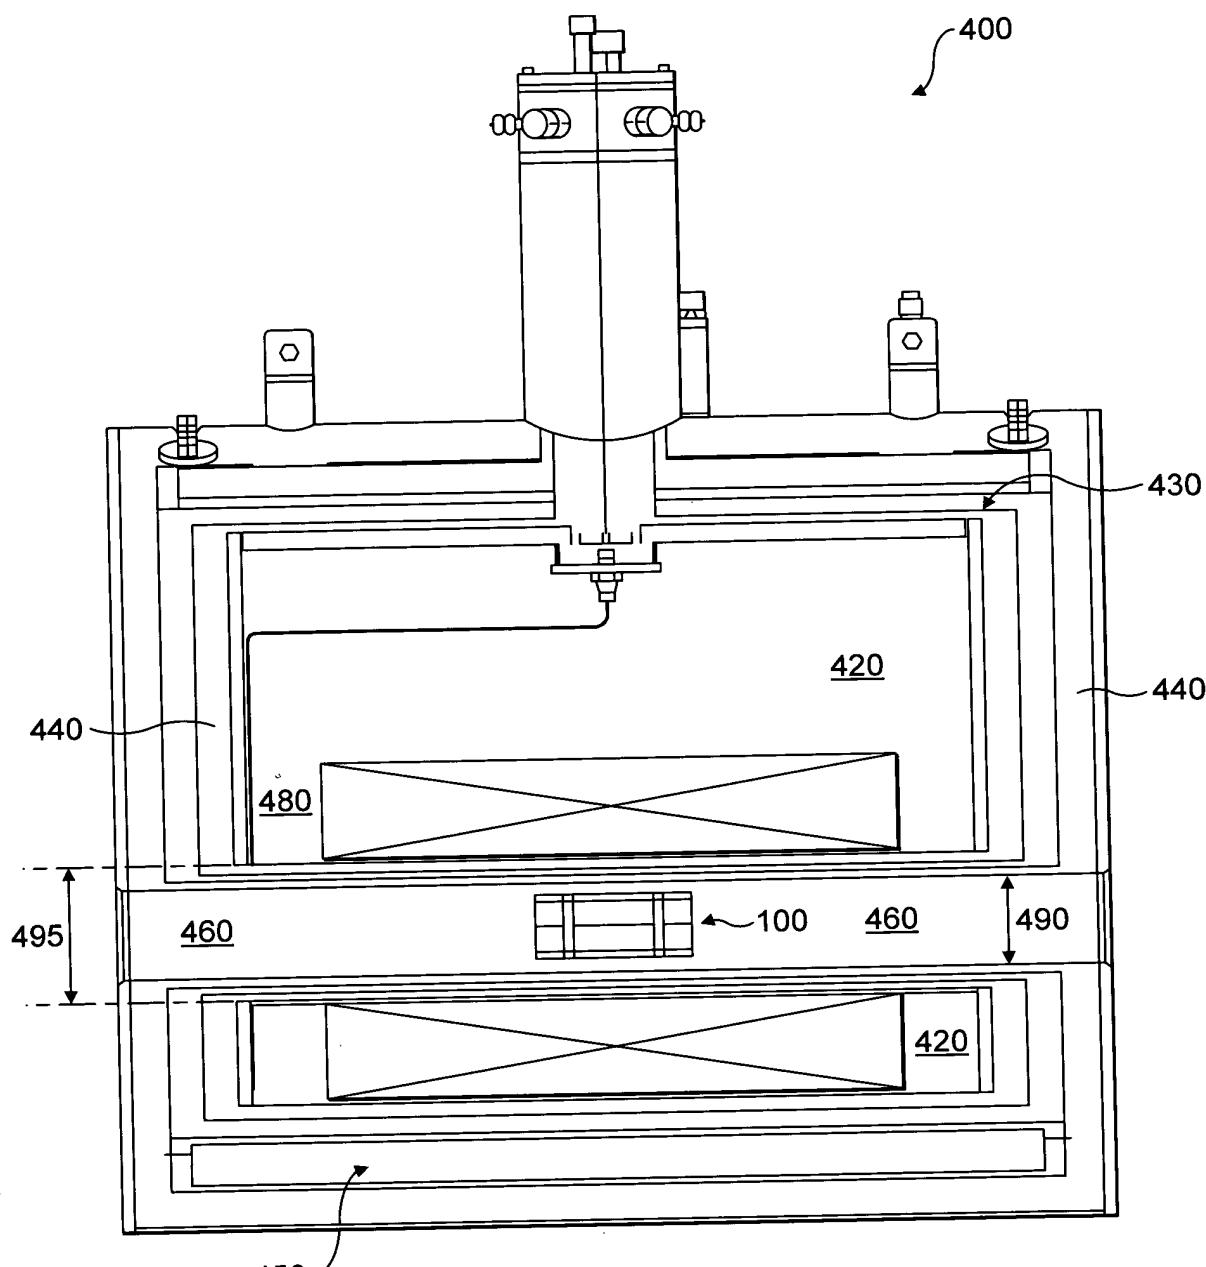


FIG. 4

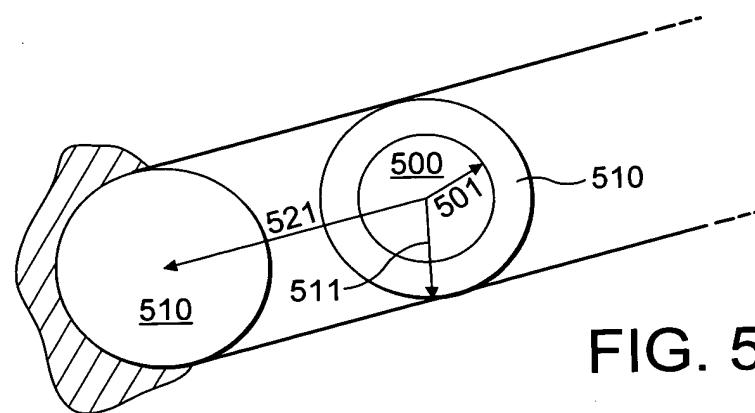


FIG. 5

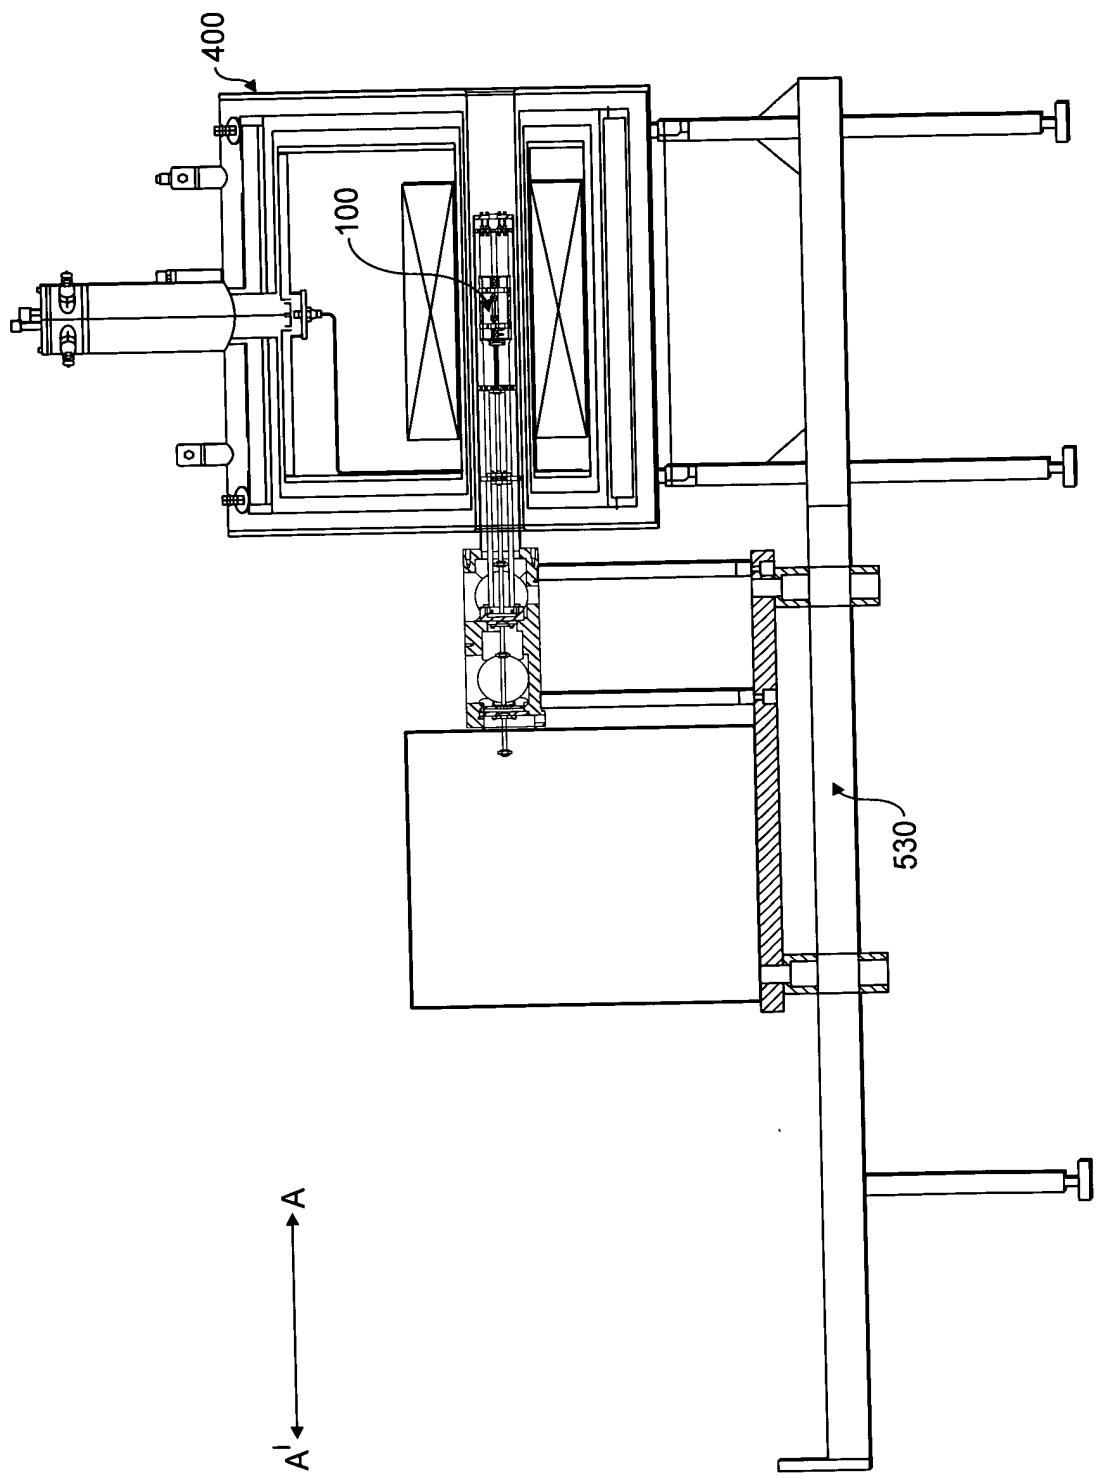


FIG. 6a

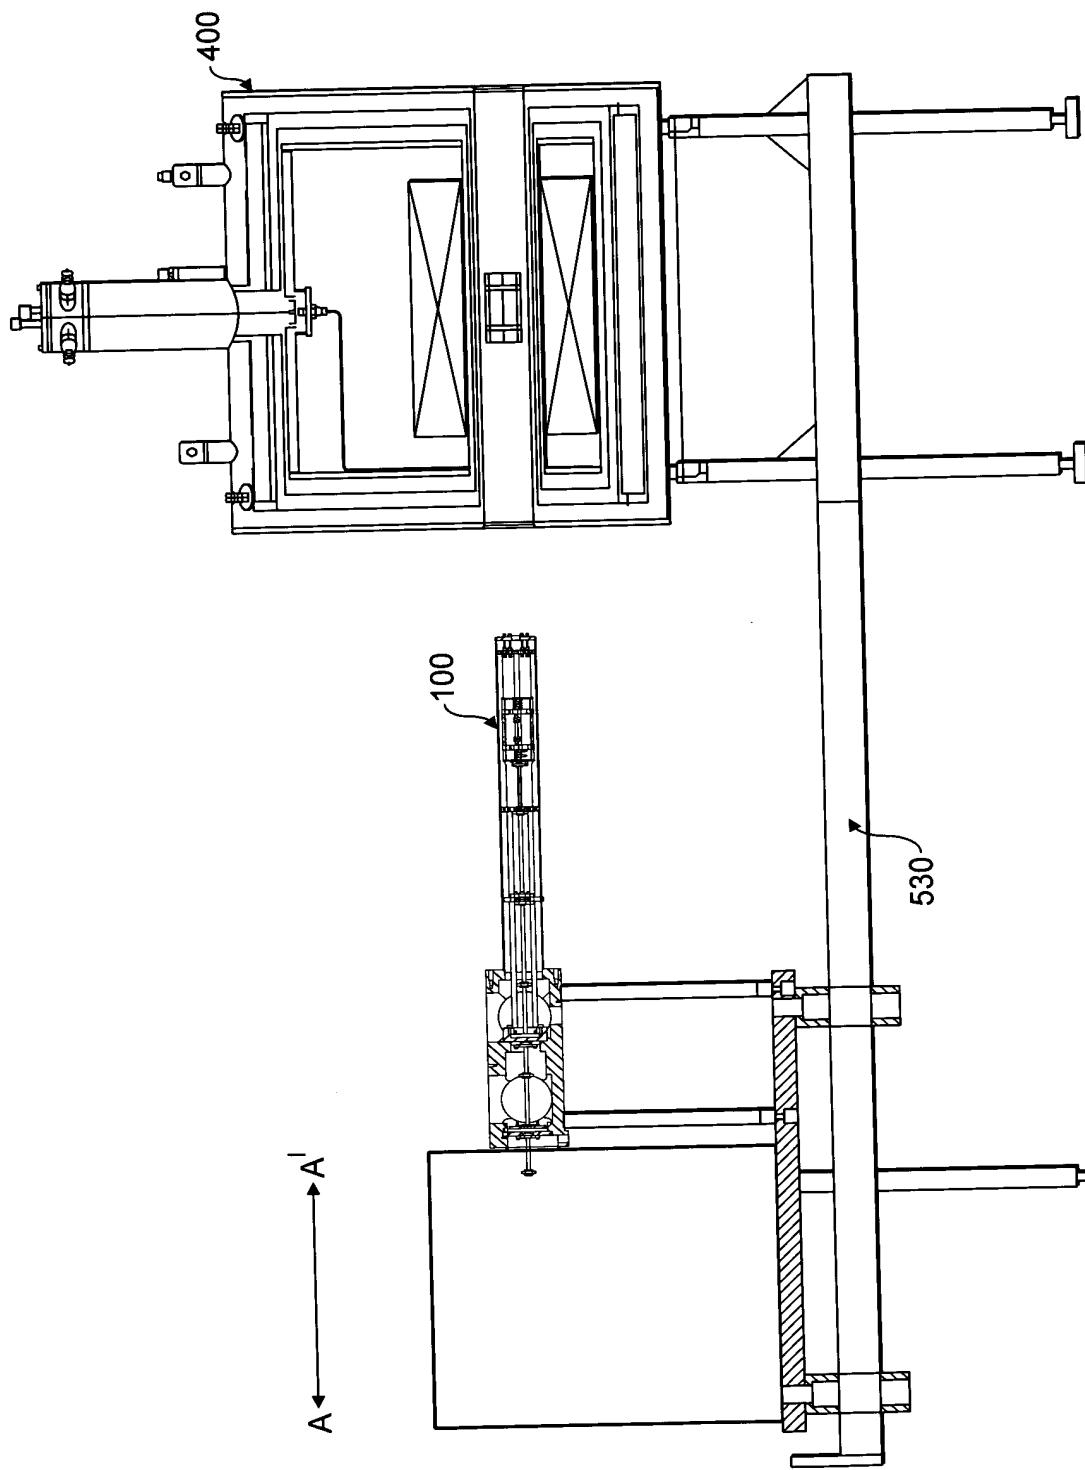


FIG. 6b

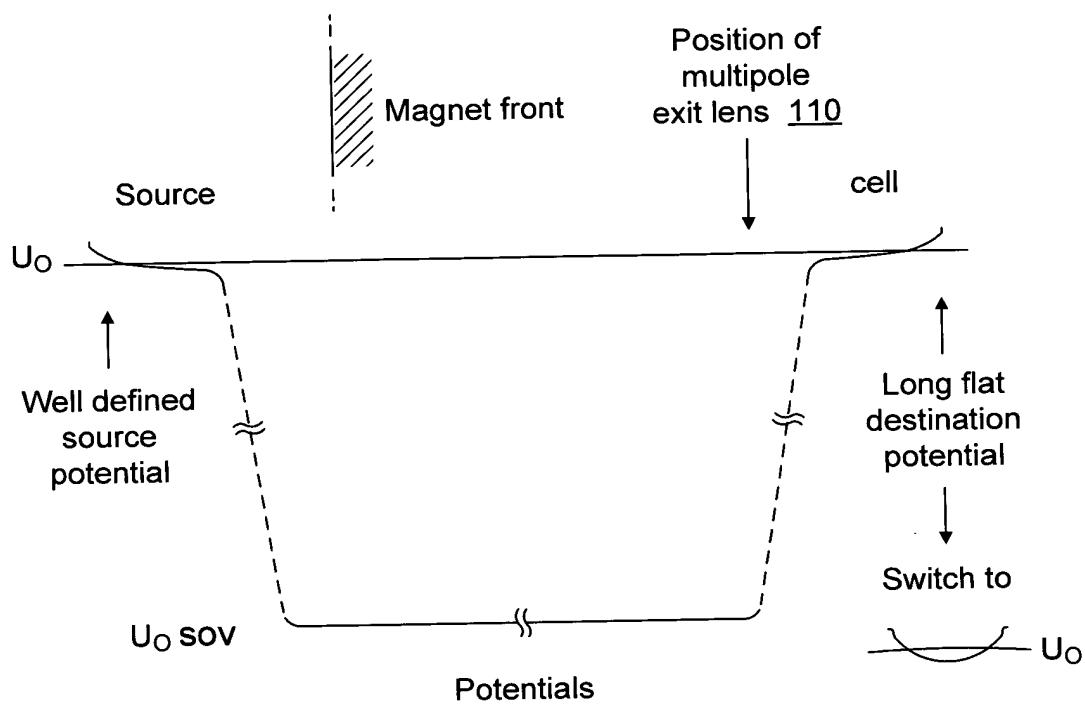


FIG. 7